

Design of Digital Percolation Meter to Determine The Water Absorption Rate (The Technology of Environmental Health)

I Dewa G. H. Wisana¹, Winarko², Budi Pramono³

¹Electromedical Engineering Department, Health Polytechnic of Surabaya, ²Health Environmental Department, Health Polytechnic of Surabaya, ³Health Environmental Department, Health Polytechnic of Jakarta II

Abstract

Several studies have report that a percolation test suits are required for planning permissions for all proposed new homes which do not have access to public mains. A percolation test is a test to determine the water absorption rate of soil in preparation for the building of a septic drain field (leach field) or infiltration basin. percolation testing is simply observing how quickly a known volume of water dissipates into the subsoil of a drilled hole of known surface area. Percolation tests are conducted through experimental activities in the field as the area planned in the catchment area. Experiments were performed to determine the soil's ability to pass water expressed in minutes per inch. In general the percolation test is done manually with numerical scale observation. The problem so far is the difficulty of determining the limit of water level in the test hole because it is based on visual and wet-looking tools as a hint of water level position. Researchers see opportunities to create new tools. This exciting research is followed up by creating another tool model named "Digital Percolation Meter" which results can be read directly on the monitor screen. Research through field experiment aims to produce a digital measuring instrument that works electrically and used as a means of measuring soil absorption that has not been in the market. Implementation of the device test carried out directly through percolation tests such as procedures that have been used, namely preparing 6 holes as deep as 60 cm and saturated through filling holes with water for 24 hours. This way to get the condition of the land as if it was like the condition at the height of the rainy season. The measurement result of Percolation Meter Digital is compared with the result of measurement of manual percolation test method that has been used, to get the number of soil impregnation. Both measurements were analyzed through the AUC curve. Testing data delivery time (ON) at different levels of recharge levels conducted at a height of 1 inch, 3 inch and 5 inch, the researchers put the initial sensor at the top. Then the timing results compared to using stopwatch as gold standart. Results from time data submissions show in 5 Inch and 3 inch has 100% sensitivity, and in 1 Inch level has 98%. Lower limit water level sensor using infrared and photodiode. Testing data delivery time is completed at different levels of recharge levels conducted at the level of 5 inch, 3 inch and 1 inch, Researchers put the sensor level water sensor at the bottom. The result show in 5 inch have 98% sensitivity, 3 inch has 96% and 1 inch has 92% Sensitivity.

Comment [U1]: abstract is written not in italics

Keywords: Percolation, Soil, absorption time, Water Level

Introduction

Percolation Test is a method of measuring the power of soil absorption to obtain percolation rate in an area that will be used as infiltration. The percolation test is carried out through experimental activities in the field as the planned area for a recharge area, ie an experiment conducted to determine the soil's ability to pass water expressed in units of minute per inch (minute / inch)⁽¹⁾.

The problem in the trial is the difficulty of determining the limit of the water level in the test hole because it is based on visual and wet-looking tools as a water level position. The wet sections are still influenced by the capillary system of objects used as a measuring instrument so that it still contains the risk of error. Required tools that can help the accuracy and ease in the process of measurement that until now does not exist.

Percolation Meters in the form of tubes still have weaknesses if the meter does not concentrate on watching the water level drop on the monitor tube, so it needs to develop better tools and work automatically. Digital Percolation Meters in the study are designed to facilitate their use as soil remapping devices so they can be used as a tool to assist in the measurement of absorption numbers in the field and automatically. The result of digital percolation is read on the monitor screen. Digital Percolation Meter is a new tool that has not existed so far.

Research conducted by san ming ke and hau Ding Ku in 2012 under the title "Research on percolation model and criticality of seismicity" has developed analog percolation technique to transmit time monitoring information still using stopwatch. The system only monitors water absorption and records it manually only⁽³⁾.

Subsequent research was conducted by Dubber D and L Gill and in 2013 made a study entitled "EPA research options for low-percolation sites" that led to a percolation system on slowly groundwater soil with manual monitoring.


This system will monitor percolation continuously to monitor the movement of the soil with slow percolation⁽⁷⁾.

By looking at other percolation system opportunities that have been further developed by Legger researchers in 2014 taking a research entitled “Percolation and Universal Scaling in Composite Infiltration Processing” introduced a percolation system to perform universal data analysis. Two devices are used into the ground area to create a percolation system⁽⁵⁾.

With the limitations on the percolation system that is only developed manually on one time monitoring alone, then in this study, researchers will make a Digital Percolation Meter. Digital percolation meter can detect soil absorption in real time and send information to microcontroller system. Digital Percolation meter not only monitors the conditions of the recharge time but also gives a decision when the system should stop so that the time of soil absorption can be known with certainty.

Materials and Method

The percolation process is the process of moving water through the soil profile due to gravitational forces. Calculation of time data to calculate automatically when water starts to drop digitally using arduino microcontroller system. Arduino Uno is a microcontroller based board on ATmega328. Arduino Uno is built from every component needed to support the function of a microcontroller. Arduino microcontroller system uses two sensors. This first sensor is used to set the start time to be calculated when the water starts to drop from the starting point until the time will stop at the last point indicated on the second sensor when the water has decreased. The sensor will detect the movement of water into the ground through the cracks and pores of the soil and rocks towards the groundwater level. When the second sensor then the water can move due to capillary action or water can move vertically or horizontally below the soil surface until the water reenter the surfacewater system see in figure 1 (A).

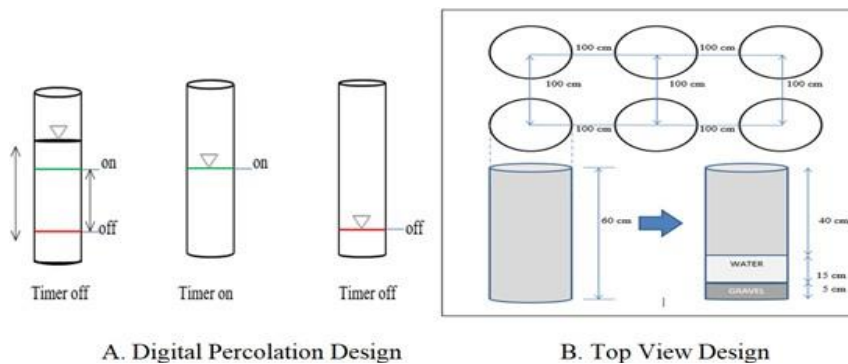

A. Digital Percolation Design

B. Top View Design

Comment [U2]: complete the image title


The experiment was carried out in a location to be used as a recharge area by making 6 holes with a diameter of 10 - 30 cm or a cube with a side of 10 - 30 cm as deep as 60 cm with a distance between holes 100 cm as shown in the figure 1 (B). The decrease of water in the test hole after 12 - 24 hours of water baiting remains, then the water level is increased to 15 cm above the surface of the gravel and then calculated the time required to absorb water 1 inch up to the last experiment, since the last result is used as reference Determination of the amount of absorption rate.

Benefits of percolation research of digital meters as soil catchers can be used to measure soil absorption values in the field. In addition to measuring soil recharge rates it also makes it easier for construction workers to determine the value of soil recharge to be constructed. This soil recharge value is used as one of the decisions to establish a building.

Findings

The water level circuit design uses infrared and Photodiode modules that use standard infrared protocols and a voltage requirement of 3.3 V. Photodiode is an easy-to-use SPP (Serial Port Protocol) module for serial wireless communications converting serial port to Bluetooth. Infrared uses bluetooth modulation V2.0 + EDR (Enhanced Data Rate) 3 Mbps by utilizing radio wave frequency 2.4 GHz.


The signal conditioning circuit is output after the capacitor. The output signal after the capacitor is at the ground point, because the signal has passed the high pass filter circuit and passed through the capacitor. The function of the high pass filter circuit is to pass the frequency above the cut off frequency (0.7 Hz) and suppress the amplitude of the frequency below the cut off. The function of the capacitor is to hold DC signals (DC blocking), so that the DC voltage that appears along with the sensorship results can be suppressed. Output that comes out of the sensor still can not be determined results of infrared sensorship, it needs to be strengthened in order to be legible. Notch Filter circuit module is a filter that has characteristics will hold the signal with a frequency corresponding to the cut off frequency of the circuit and will pass signal with frequency outside the cut off frequency of the filter circuit either below or above the cut off frequency of the filter circuit.

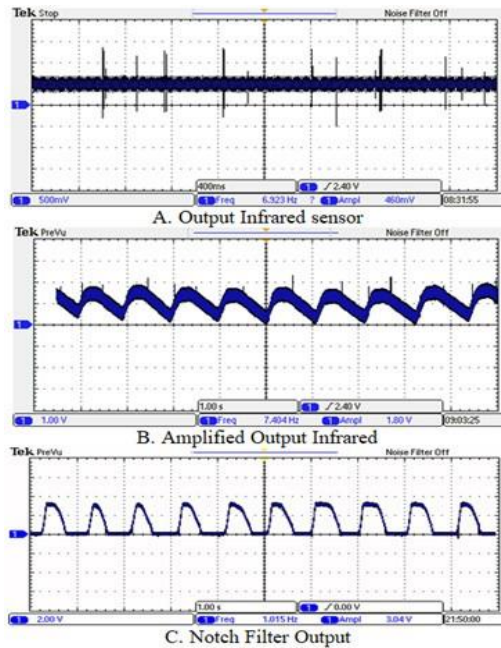

Comment [U3]: complete the image title

Software design Serial data transmission. Serial data transmission is used to see if the data transmission speed capability can match the connected hardware. This affects the results of sending data serially.

To use the serial communication function it must initialize first that the default serial starts with baudrate 9600 on the Rx / PD0 and Tx / PD1 pins by adding the script; `Serial.begin (9600)`; To transmit data is used function `Serial.print ()` / transmit data on pin Tx / PD1 microcontroller to Rx Bluetooth and to receive data using `Serial.read ()` / receive data from Tx bluetooth pin to Rx / PD0 microcontroller. With the amplitude still difficult to comparator then the signal is reinforced to be more sensitive.

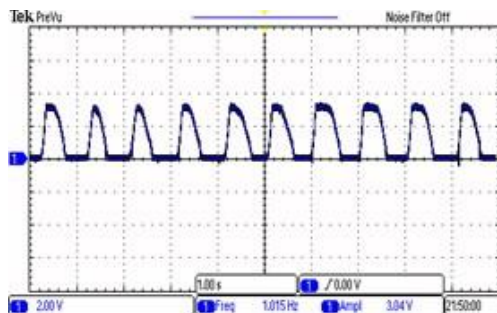


Comment [U4]: complete the image title

Data Reception software design Creating a connection path with `InputStream` to insert or store data in byte data. `InputStream` function of entering the received byte data through bluetooth. `MmInputStream` as a variable that will later to accommodate data from `tmpIn`. The connection path using the bluetooth device is declared with the `BluetoothSocket` function. `tmpIn (InputStream tmpIn = null)` is a variable from `InputStream` to set the path of `tehubungnya` sensor device to receive byte data. `tmpIn (tmpIn = socket.getInputStream ())` will be used as a temporary device to get / hold the byte data that has been entered on `InputStream`.


If there is already data or value, then the data in `tmpIn` will be stored on `mmInStream` variable that has been specified above (`mmInStream = tmpIn`) to be processed in processing convert data byte into data string for data can be displayed.

Discussion

Analysis percolation meter research uses two water level sensors that are level sensors to initiate calculations and level sensors for stopping water levels. The Water Level Sensor starts this calculation which will then read the initial time value of the existing water level. Excess use of infrared water level sensor and Photodiode is a small form with a high level of accuracy. Additional circuit using SMD chips. These chips are selected because they have several advantages such as the form of a small chip, lightweight, low power.



A. Top View Percolation Digital

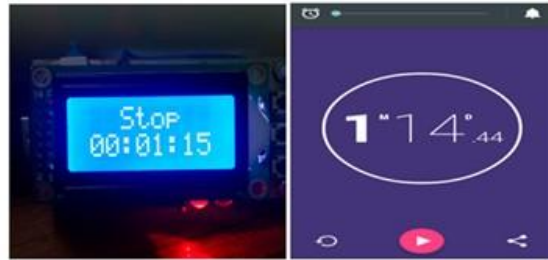

B. Data Time Compare With Stopwatch

The stopwatch is used as a standard Gold on the water reduction from the top-level sensor to the lower-level sensor on the digital meter percolation system. The data will be compared between the data received in the module display with the data transmitted to the microcontroller. At the same time data is also viewed using Stopwatch.

Testing data delivery time (ON) at different levels of recharge levels conducted at a height of 1 inch level, 3 inch and 5 inch, the researchers put the initial sensor at the top. Then the timing results compared to using stopwatch as gold standardnya. The results of time data transmission can be seen in the table 1.

Test Data ON	Level 5 inch	Level 3 inch	Level 1 inch
Stop watch (GS)	50	50	50
Data Time On	50	50	49
True Positive	50	50	49
False Negative	0	0	1
False Positive	0	0	0
Sensitivity (%)	100	100	98

From the results of table 1 it appears that the sensitivity at Level 5 inch is worth 100%, then after the level is lowered to 3 inch the sensitivity value remains 100%. At the water level lowered to 1 inch the sensitivity value drops to 98%.

Test Data Off	Level 5 inch	Level 3 inch	Level 1 inch
Stop watch (GS)	50	50	50
Data Time On	49	48	46
True Positive	49	48	46
False Negative	1	1	3
False Positive	0	1	1
Sensitivity (%)	98	96	92

Table 2 shows that the sensitivity of lower level sensor at 5 inch level is 98%, then after the distance is lowered to 3 inch the sensitivity value decreases to 96%. At a distance lowered to 1 inch the sensitivity value drops to 92%.

Conclusion

Comment [U5]:

Comment [U6R5]: complete the image title

Comment [U7]: Complete the table title

Comment [U8]: Complete the table title

Design Digital Percolation Meter has been tested began to recharge using water-level sensor infrared- photodiode to detect any changes in water level in the recharge tube. Performance is reviewed by looking at the ability of a digital meter percolation system to be able to start calculating the time sent to the microcontroller system appropriately. The sensitivity is indicated by the ability of the program to display the data start time recharge and its changes because of the decrease of water level in the recharge tube. The program averages 99% that the on time data can be sent and received by the digital percolation system well. The average program is 95.4% that the off time data can be sent and received by the digital percolation system well.

Comment [U9]: Writing the beginning of the paragraph according to the author's guide

Recommendation:

The soil percolation test is still the most practical way to obtain a quantitative indication of the hydraulic conductivity of the subsoil. As such, it will remain a significant aspect of overall site and soil assessment practices into the foreseeable future. Thus, the ability to perform a percolation test in a manner that provides accurate and repeatable results is of paramount importance for any person engaged in the practice of evaluating soils and sites for future construction or development.

Comment [U10]: Writing the beginning of the paragraph according to the author's guide

References

1. Dubber D, Gill L. EPA research options for low- percolation sites Proceeding of the Cambridge Philosophical. 2013;53:629–641.
2. Gu HD, Chen YT. Physics of seismic gap and nonscale of focal system. In: Chen Y T edit-in- chief. Advance of Chinese Seismology Research.Beijing: Seismological Press; 2003:37–40.
3. Shan-Ming Ke, Hao-Ding Gu, Wen-Jie Zhai. Research on percolation model and criticality of seismicity Geophys J Int. 2012;100:215–220
4. Léger JM, Molina-Jordá L. Weber, Mortensen A. Percolation and Universal Scaling in Composite Infiltration Processing. Acta Geophysica Sinica. 2014;35(1):25–36.
5. Wisana IDGH. Design electronic stethoscope for cardiac auscultation analyzed using wavelet decomposition. International Journal of Applied Science and Engineering Research.2014;3(1):194-202.
6. Wisana I, Widodo T, Sjabani M, Susanto A. Identification of ST segment ECG signal using *Indian Journal of Forensic Medicine & Toxicology, October-December 2019, Vol. 13, No. 4* 1562 Degestseg wavelet detection. Int. J. Comput. Sci. Telecommun. 2012;3(9):6-11.
7. Robertson MC, Sammis CG, Sahimi M, et al. Fractal analysis of three-dimensional spatial distributions of earthquake with a percolation interpretation. J Geophys Res. 2007;100:609– 620.
8. Stanley HE. Renormalization and percolation. Advance of Physics Research. 2005;5(1):1–65.
9. Smalley JR R F, Turcotte DL. A renormalizationgroup approach to the stick-slip behavior offaults. J Geophys Res. 2009;90:1894–1900.
10. Takayasu H. Shen BM, Chang ZW. Fractal.Beijing: Seismological Press; 1989:42–63.
11. Wu ZL. Implications of a percolation model for earthquake “nucleation”. Geophys J Int. 2011;133:104–110.

I Dewa G. H
Electromedical Engineering Department, Health Polytechnic of Surabaya, Indonesia
10th October, 2019

Dear Sir/Madam

LETTER OF ACCEPTANCE

Indian Journal of Forensic Medicine & Toxicology wish to inform you that your paper titled: Designof Digital Percolation Meter to Determine The Water Absorption Rate (The Technology of Environmental Health) has been accepted by Indian Journal of Forensic Medicine & Toxicology (<http://medicopublication.com/index.php/ijfmt>) October-December 2019, Vol.13, No.4 with paper reference DOI Number: 10.5958/0973-9130.2019.00523.1

Indian Journal of Forensic Medicine & Toxicology is a double-blind peer reviewed international journal. The frequency is quarterly. It deals with Forensic Medicine, Forensic Science, Toxicology, DNA fingerprinting, sexual medicine, environmental medicine, Forensic Pathology, legal medicine and public health laws. It has been assigned International standard serial No. p-0973-9122 and e-0973-9130. The Journal has been assigned RNI No. DELENG/2008/21789. The journal is indexed with Scopus, EMBASE. The journal is also abstracted in Chemical Abstracts (CAS) database. The journal is also indexed /abstracted with many databases.

This is an open access journal which means that all content is freely available without charge to the user or his/her institution. Users are allowed to read, download, copy, distribute, print, search, or link to the full texts of the articles, or use them for any other lawful purpose, without asking prior permission from the publisher or the author. This is in accordance with the BOAI definition of open access.

Remember neither has the manuscript nor one with substantially similar content under been published nor is being considered for publication elsewhere, except as described. **The processing fees per paper is US \$ 200 excluding transfer changes.**

All payment made receipt should be email to the Society Executive Director editor.ijfmt@gmail.com . The processing fees of the accepted paper(s) should be paid through the following details and remember the cost is excluding transfer charges.

Bank details Account name - Institute of Medico-Legal Publications Pvt Ltd
Bank - HDFC Bank
Branch - Sector-50, Noida-201301
Account Number - 09307630000146
Account Type - Current Account
MICR code - 110240113
RTGS / NEFT code - HDFC0000728

The Editor in Chief and Editorial Board members of the Journal appreciate your effort on the intellectual contribution of your paper.

Thank you.

Yours faithfully,

.....
Prof. Adarsh Kumar
Forensic Medicine & Toxicology,
All-India Institute of Medical Sciences, New Delhi, India
Web: <http://medicopublication.com/index.php/ijfmt/>
E-mail: editor.ijfmt@gmail.com